

FIG. 1A-3

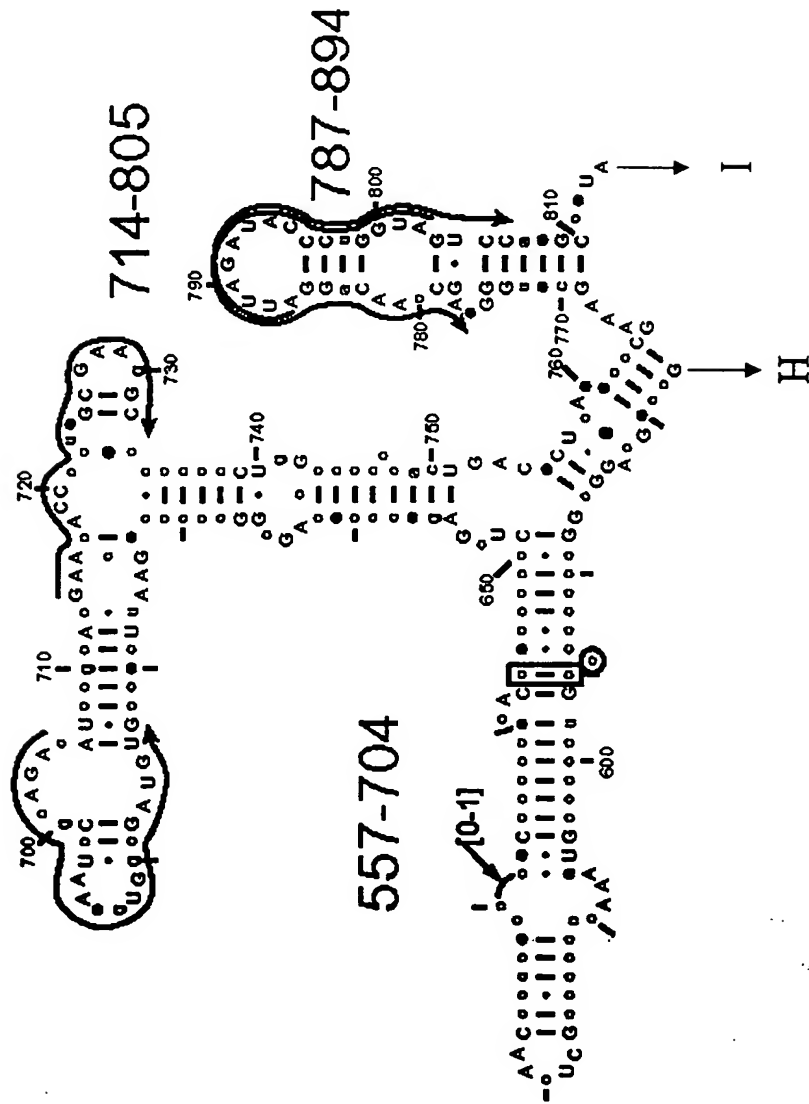
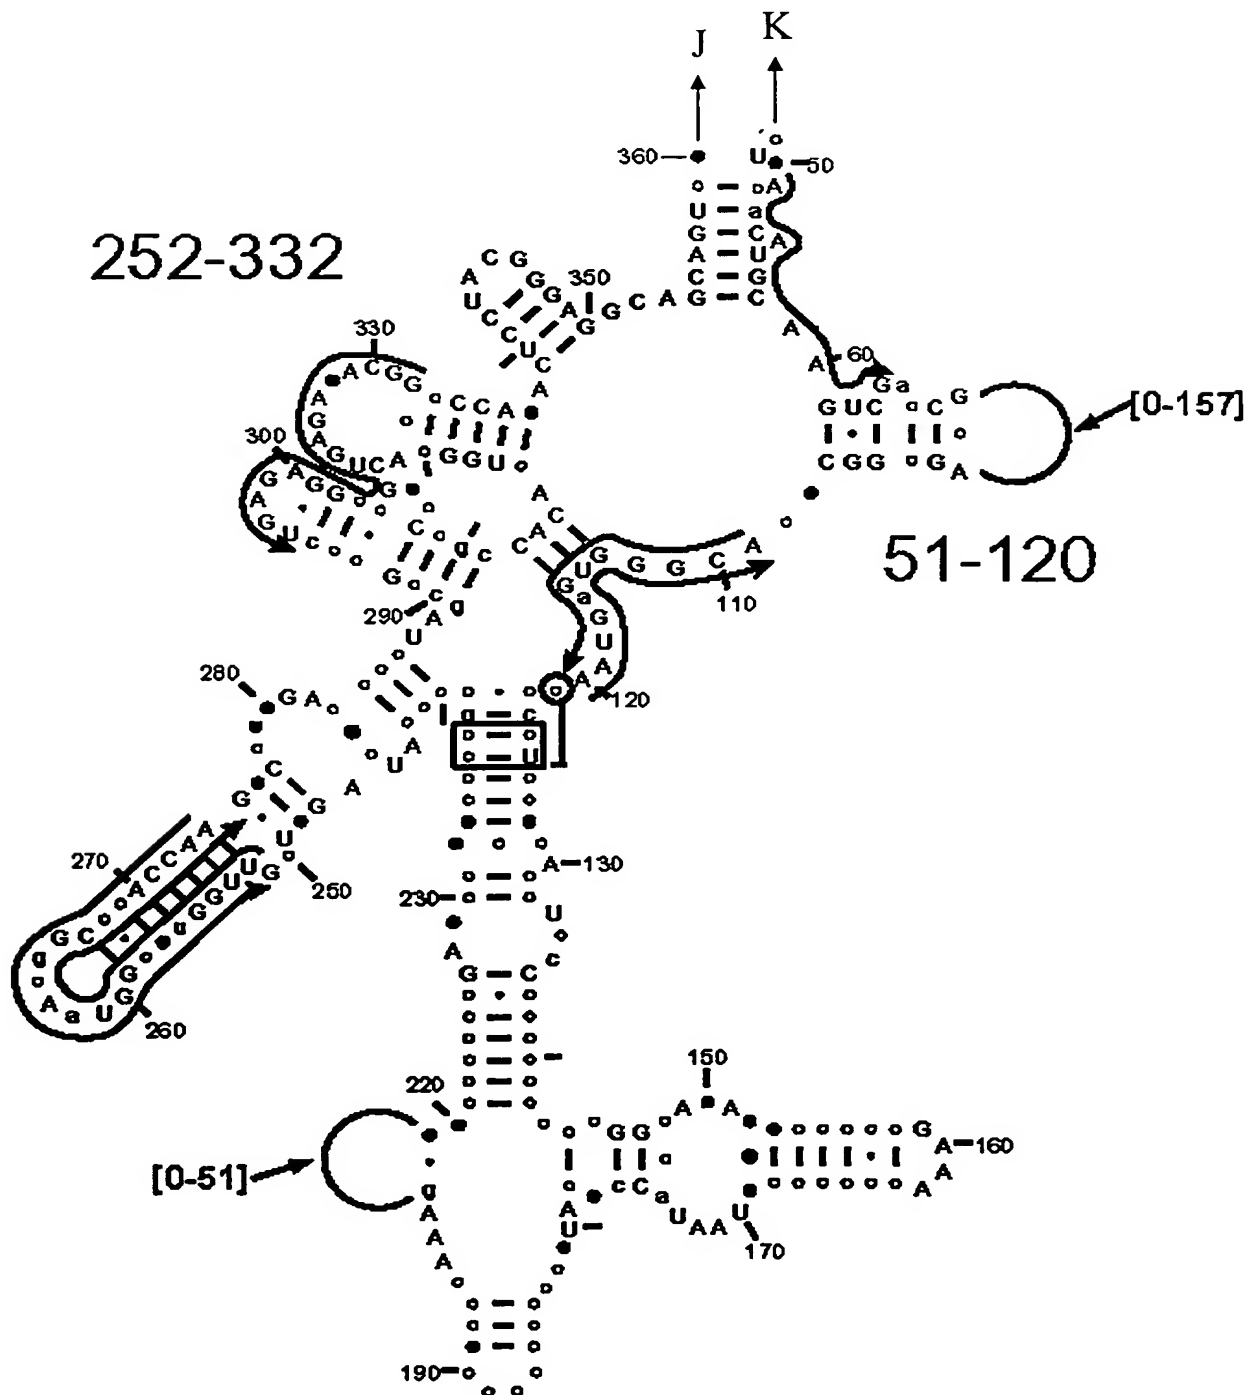


FIG. 1A-4



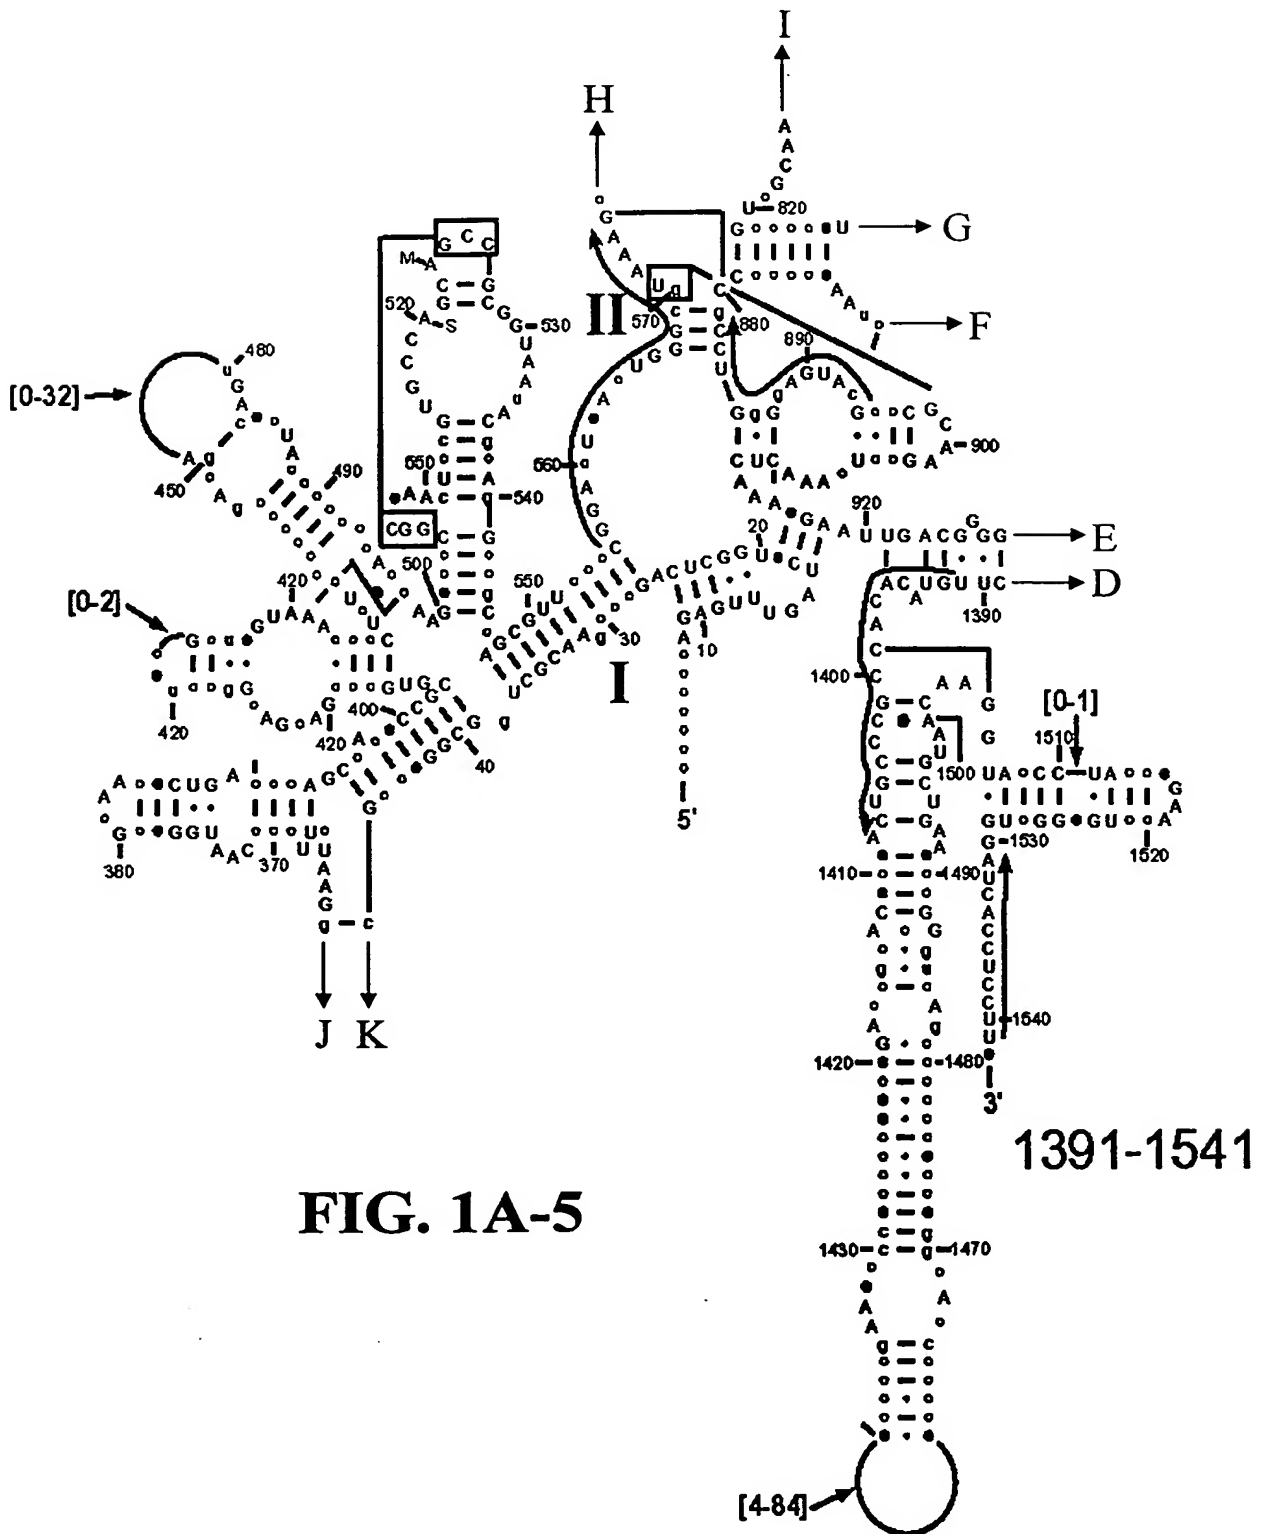


FIG. 1B

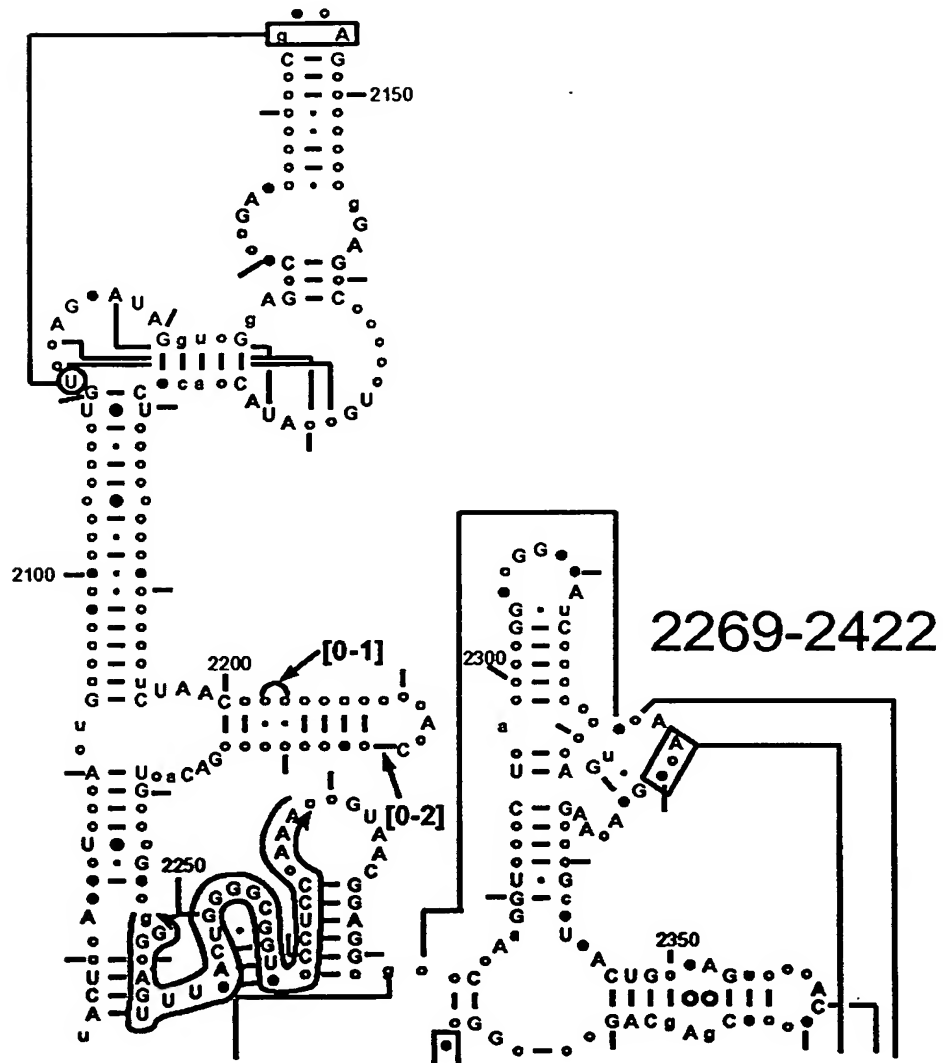


FIG. 1C

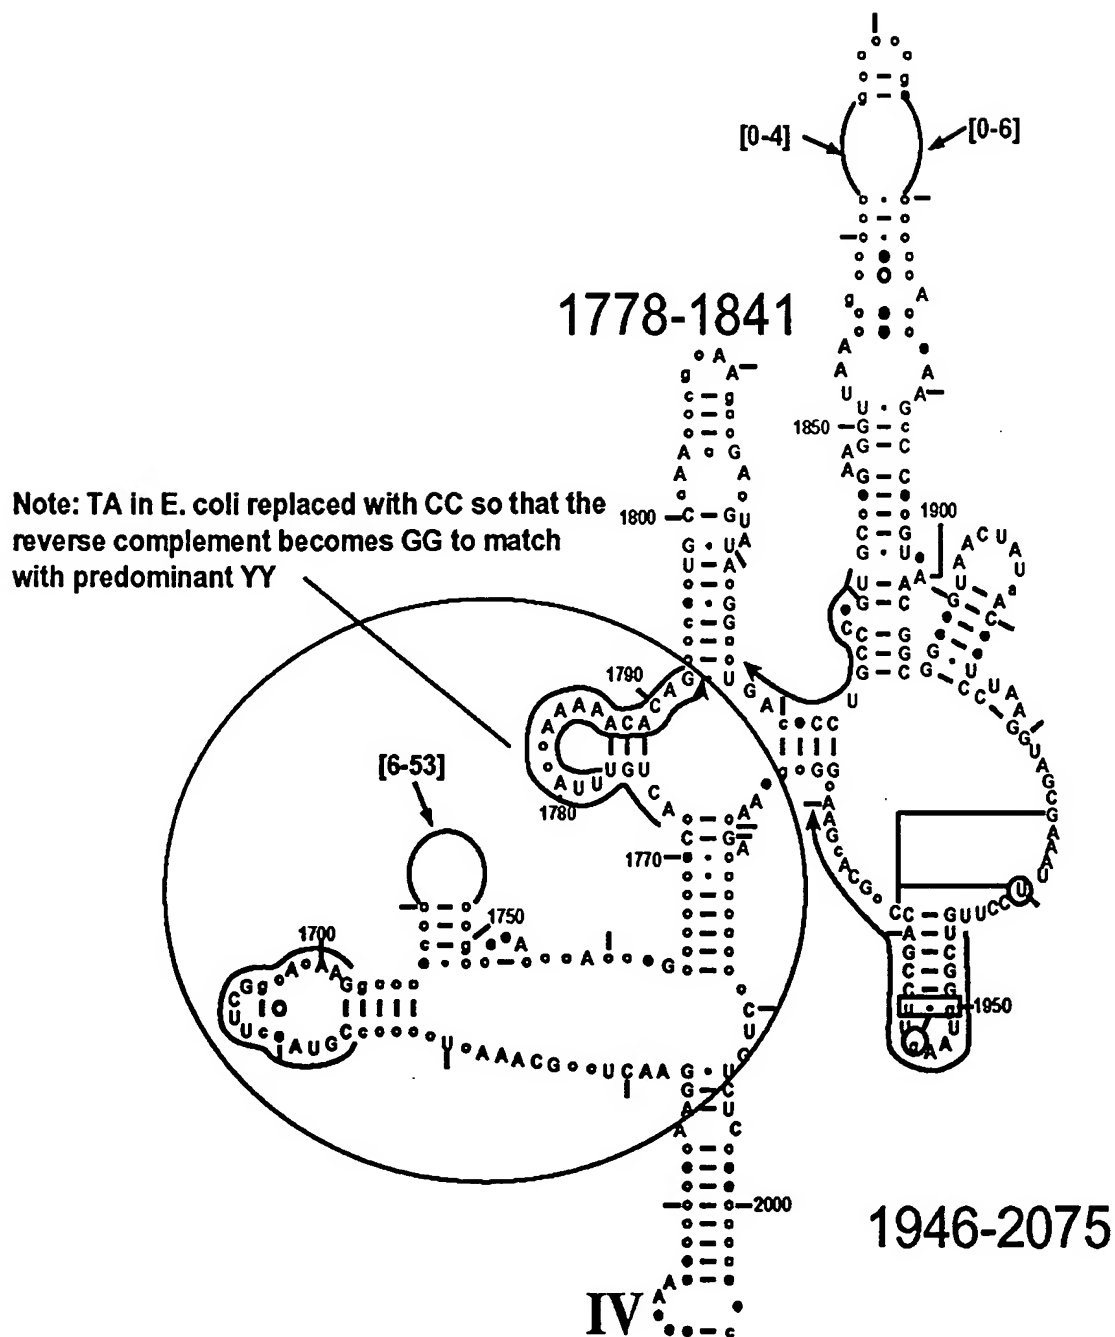


FIG. 1D

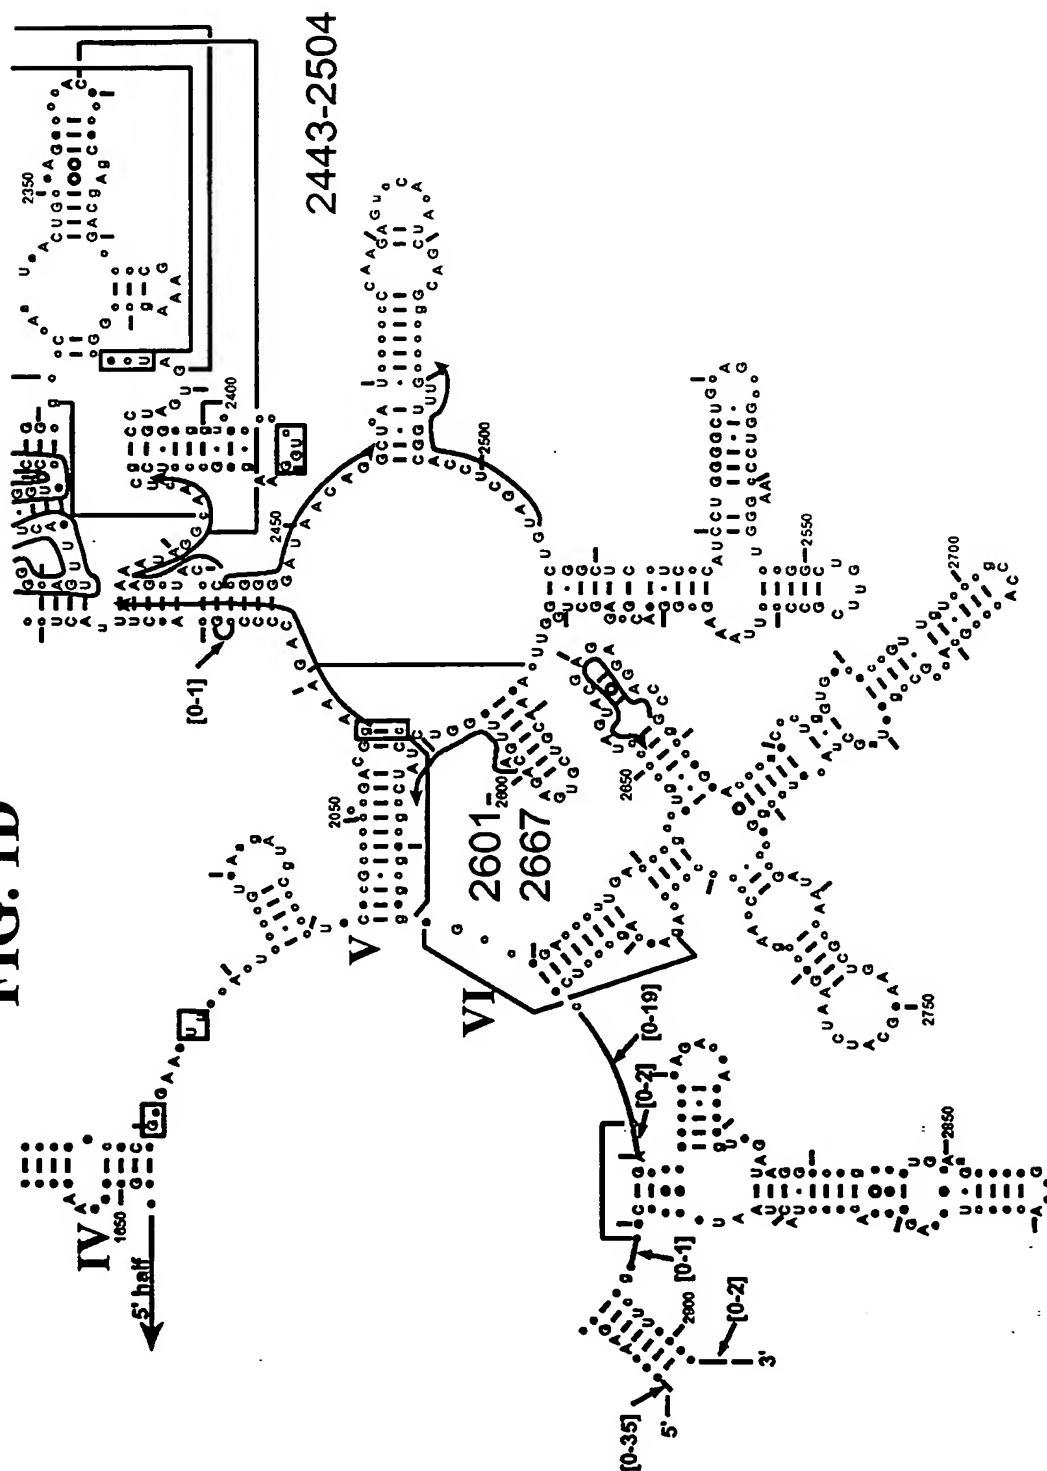
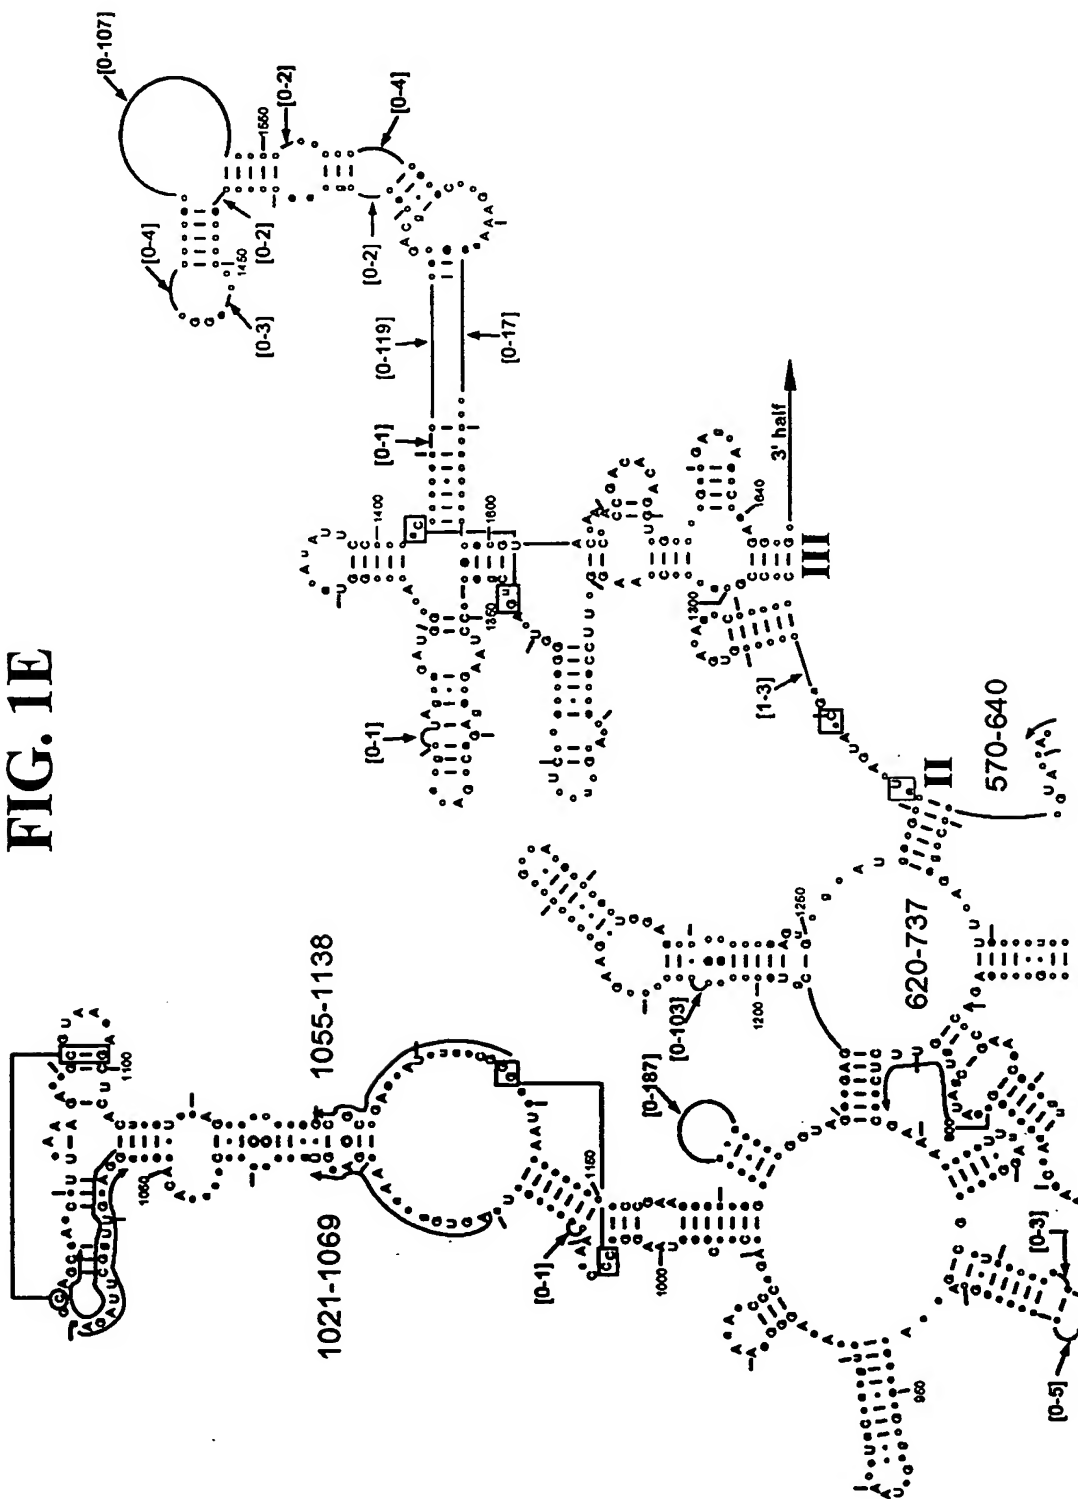


FIG. 1E



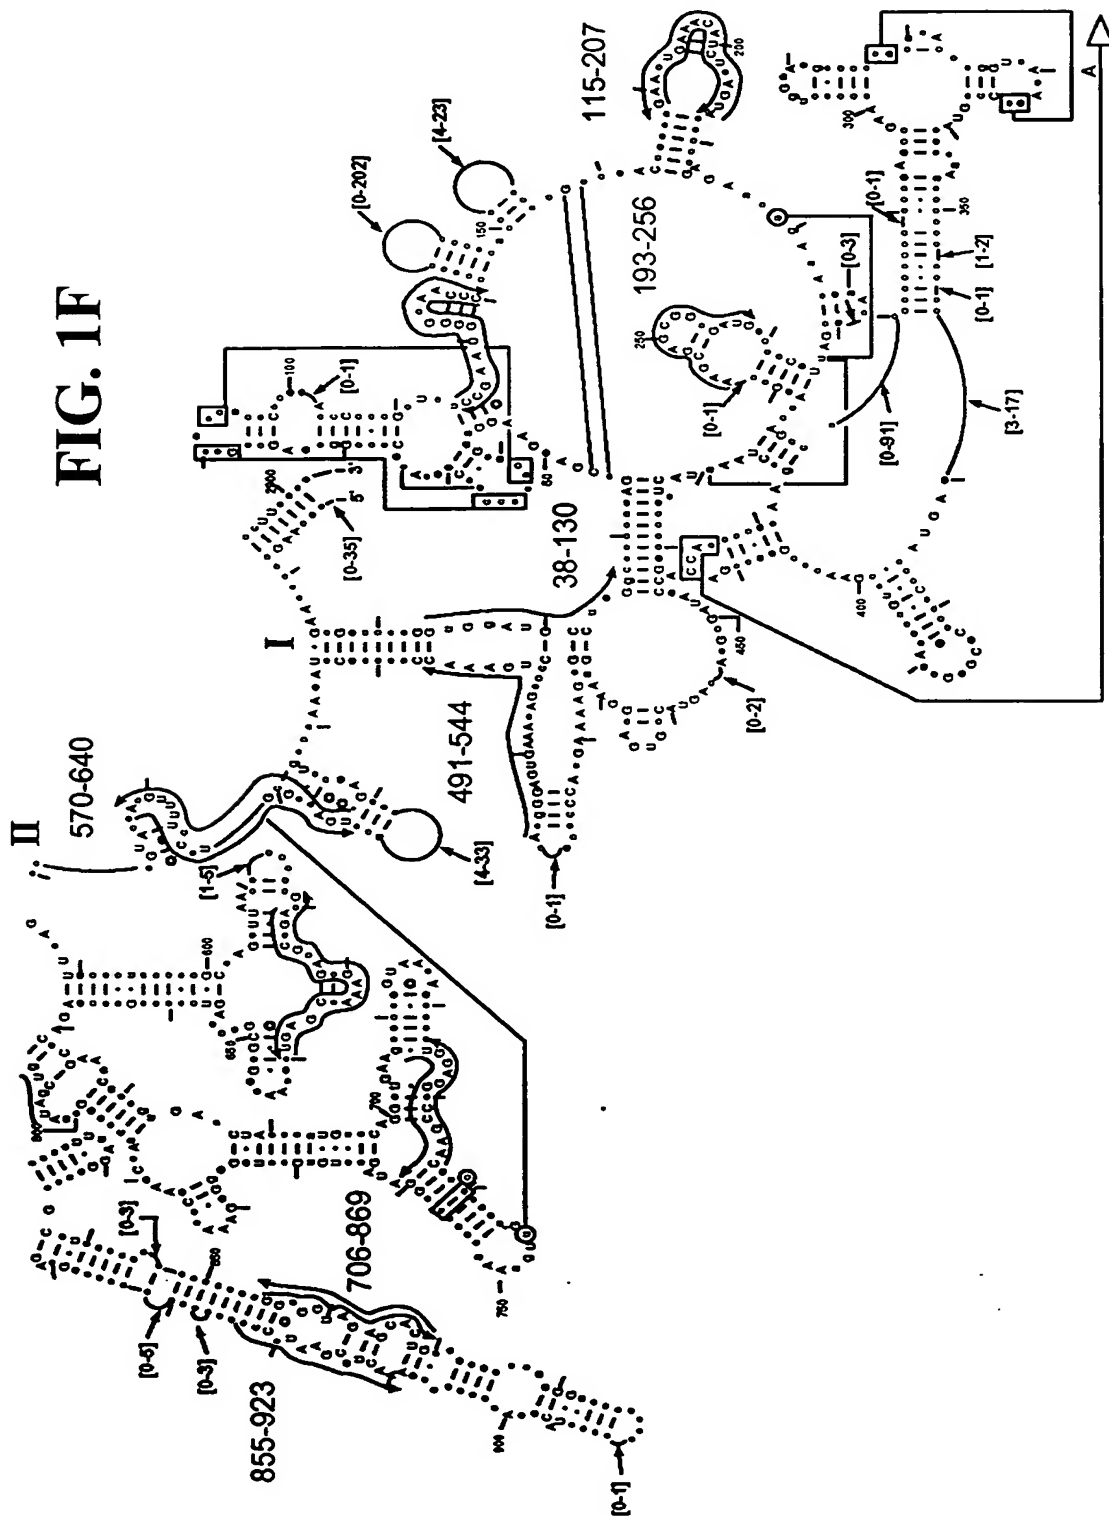


FIG. 1G

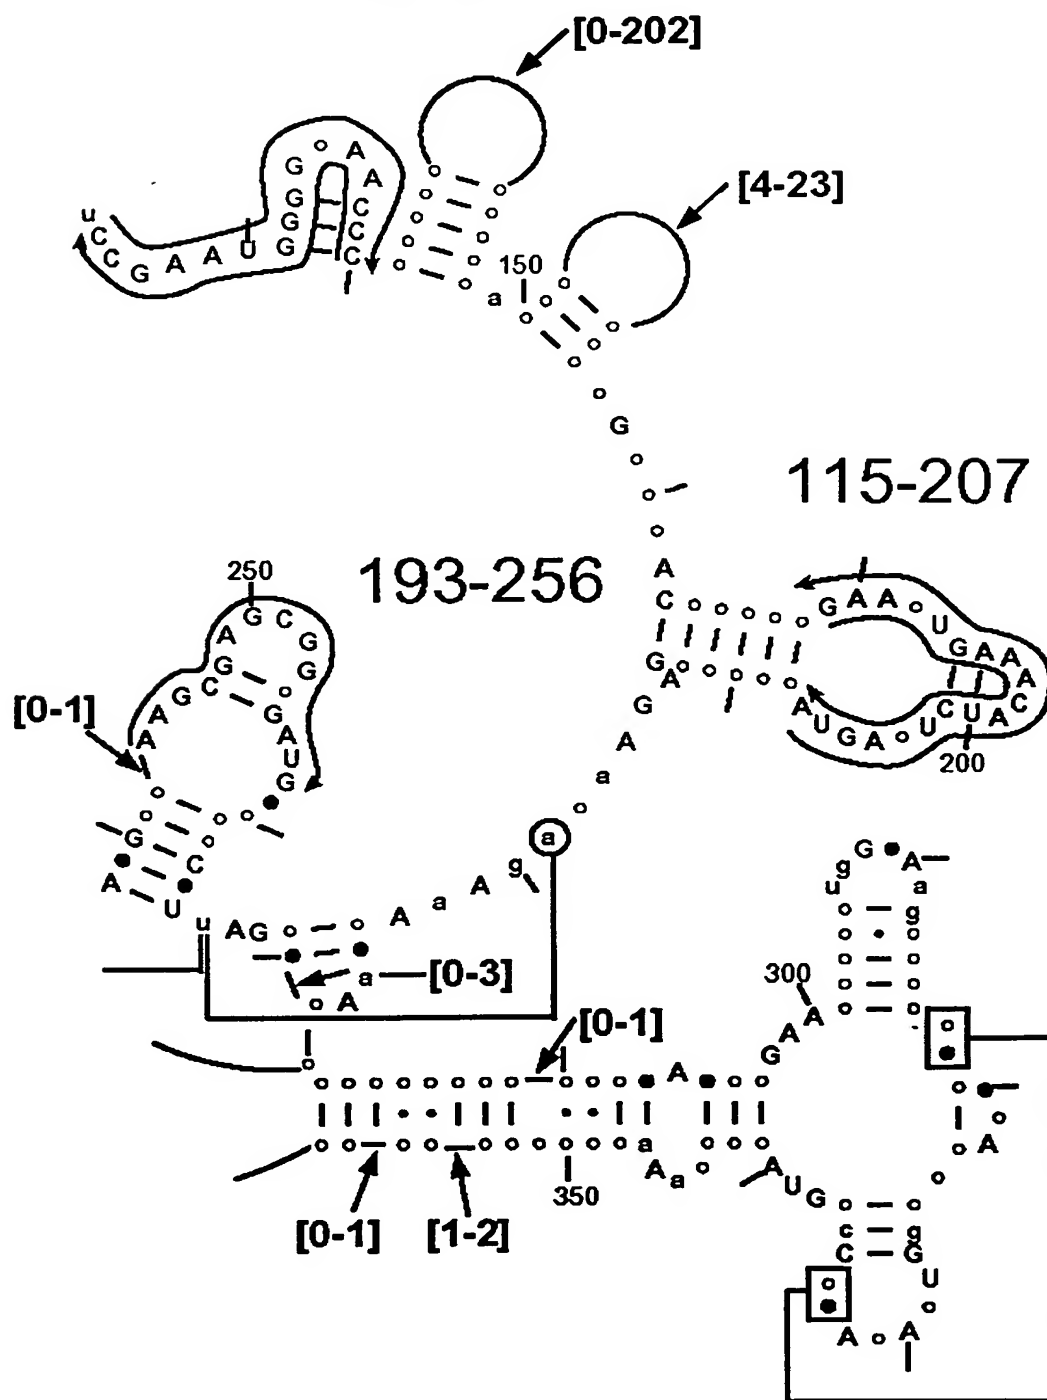


FIG. 1H

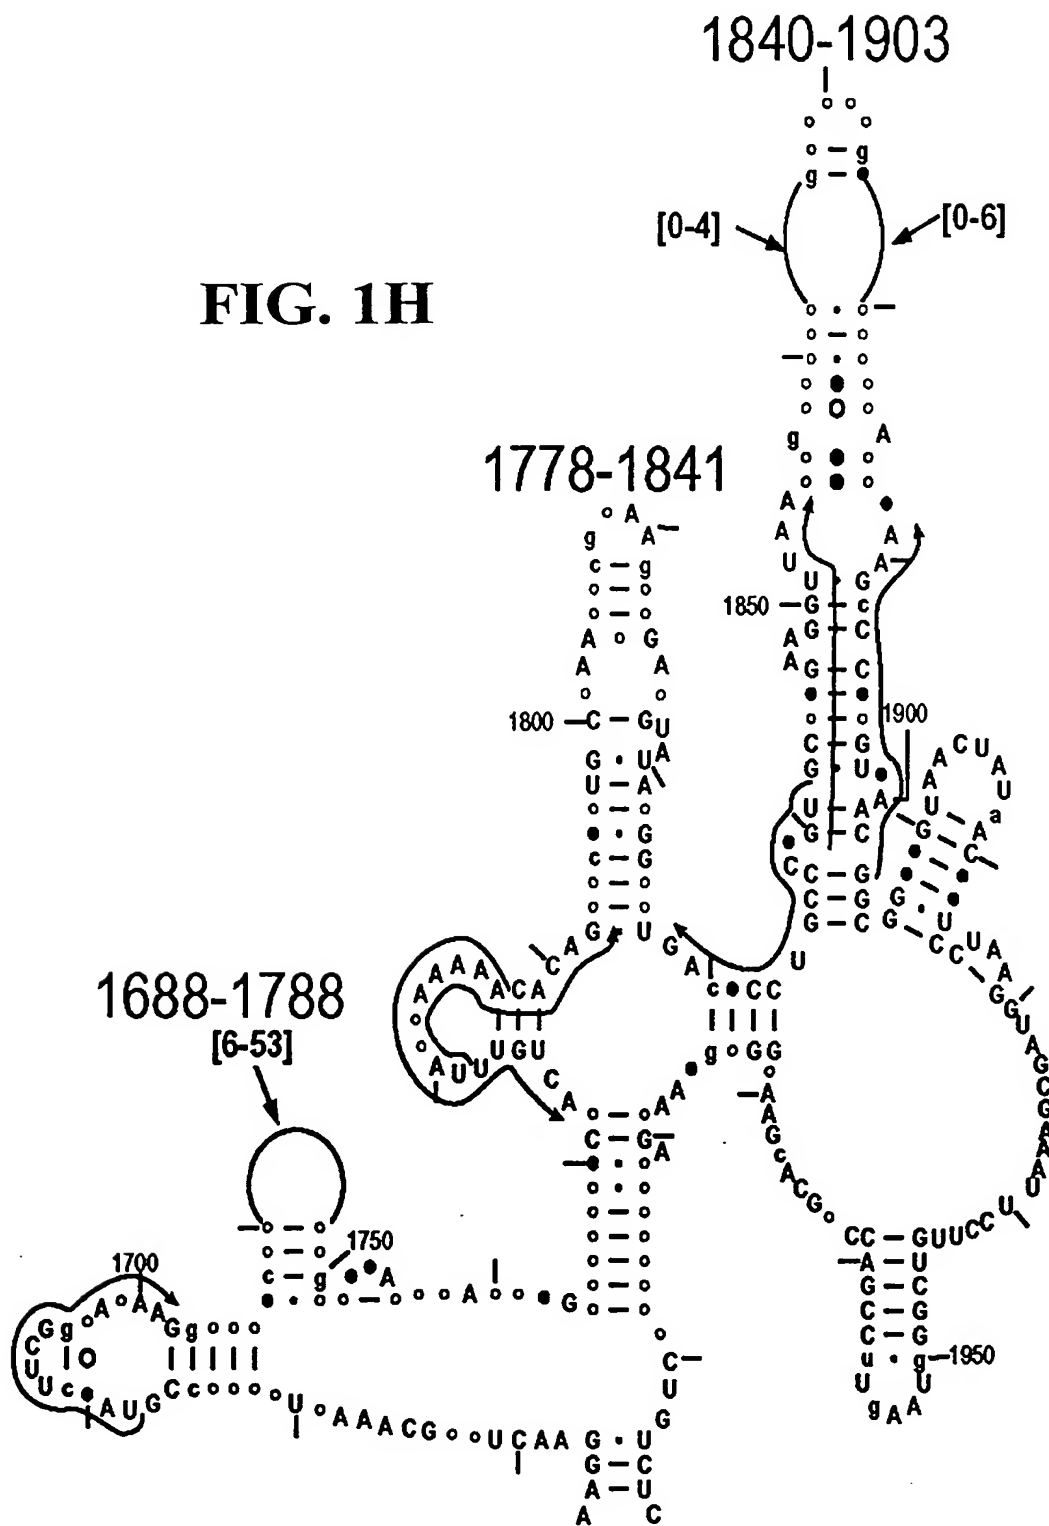


FIG. 2

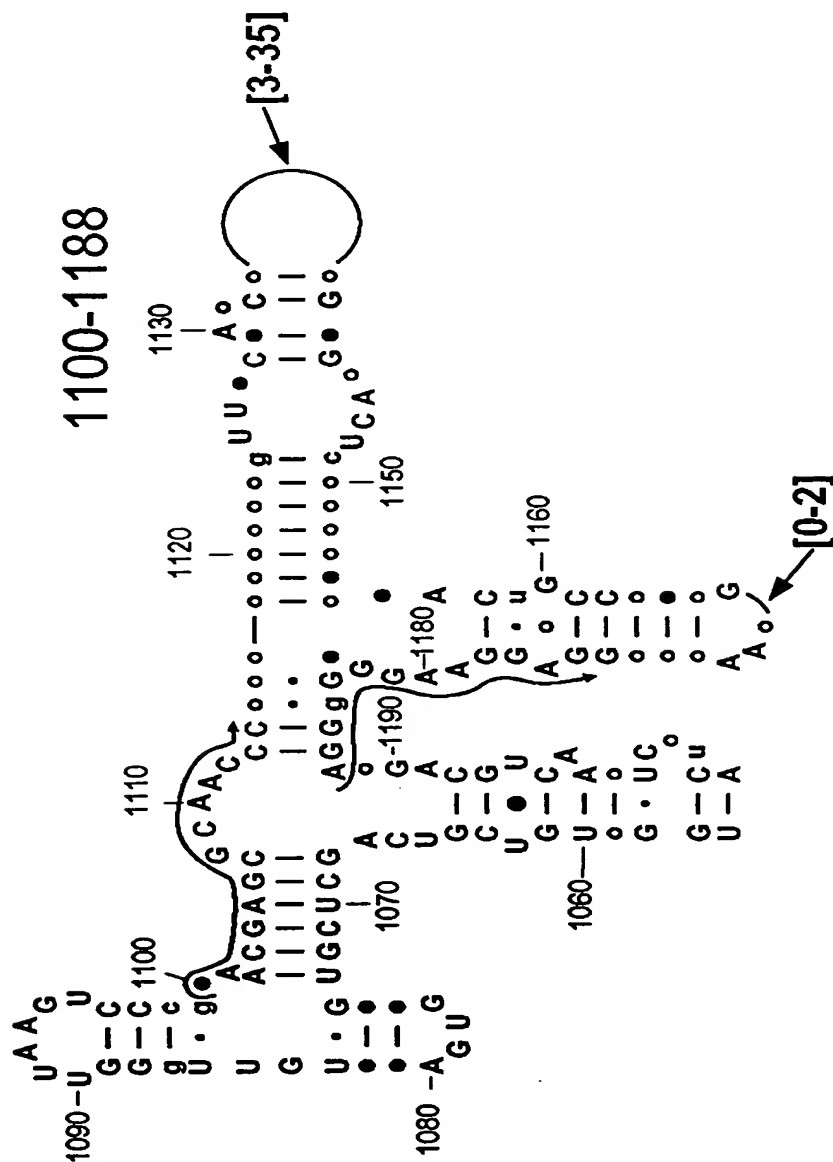


FIG. 3

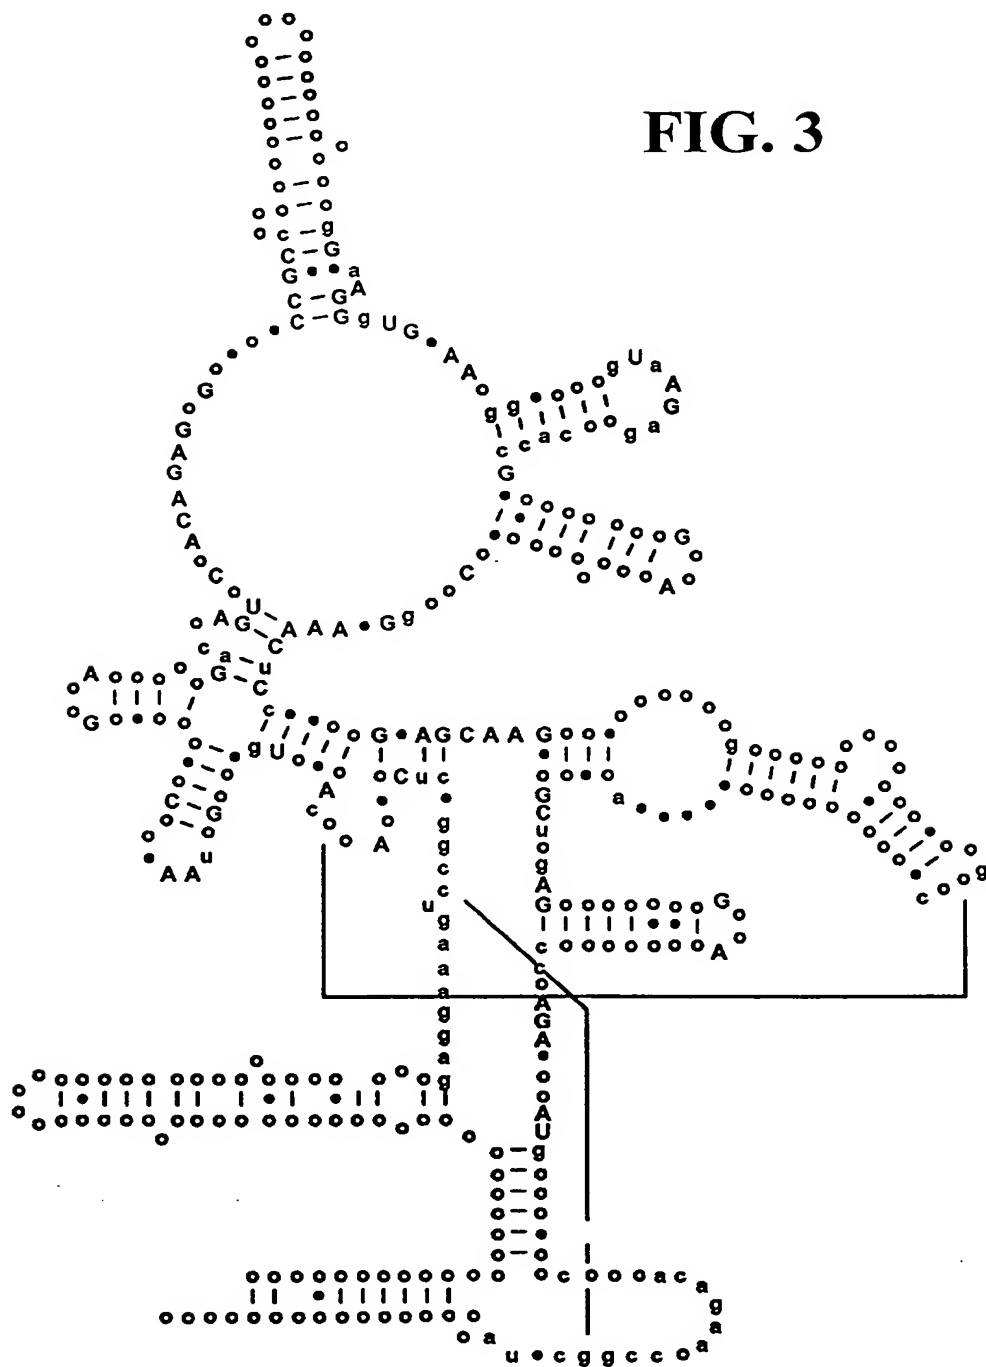


FIG. 4

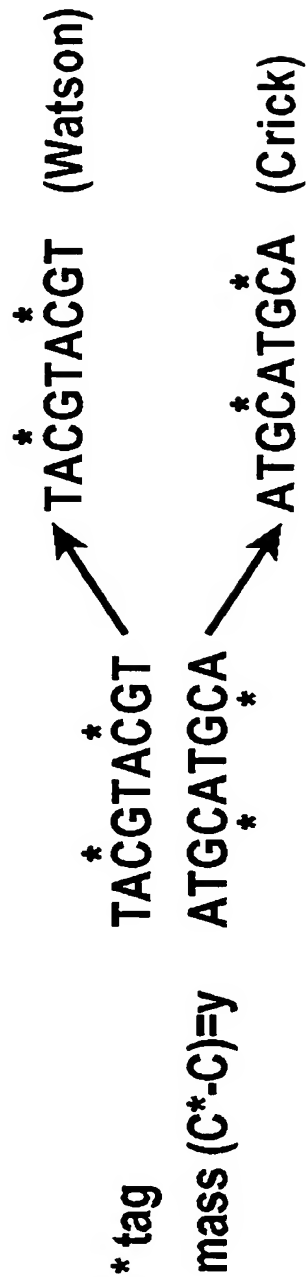
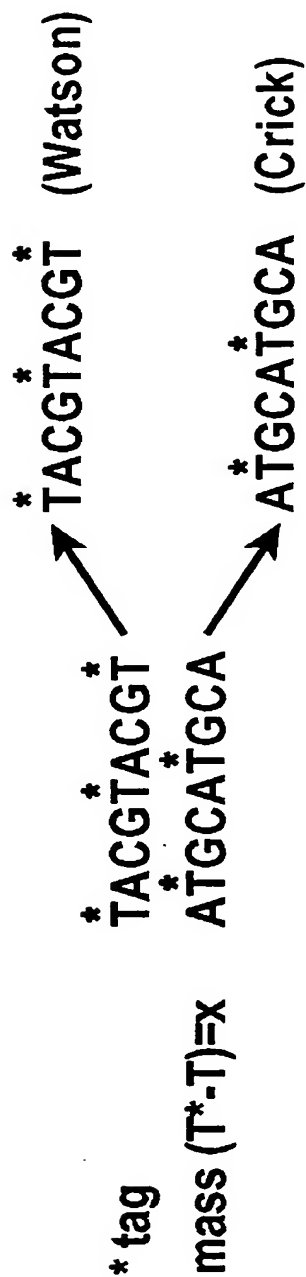


FIG. 5

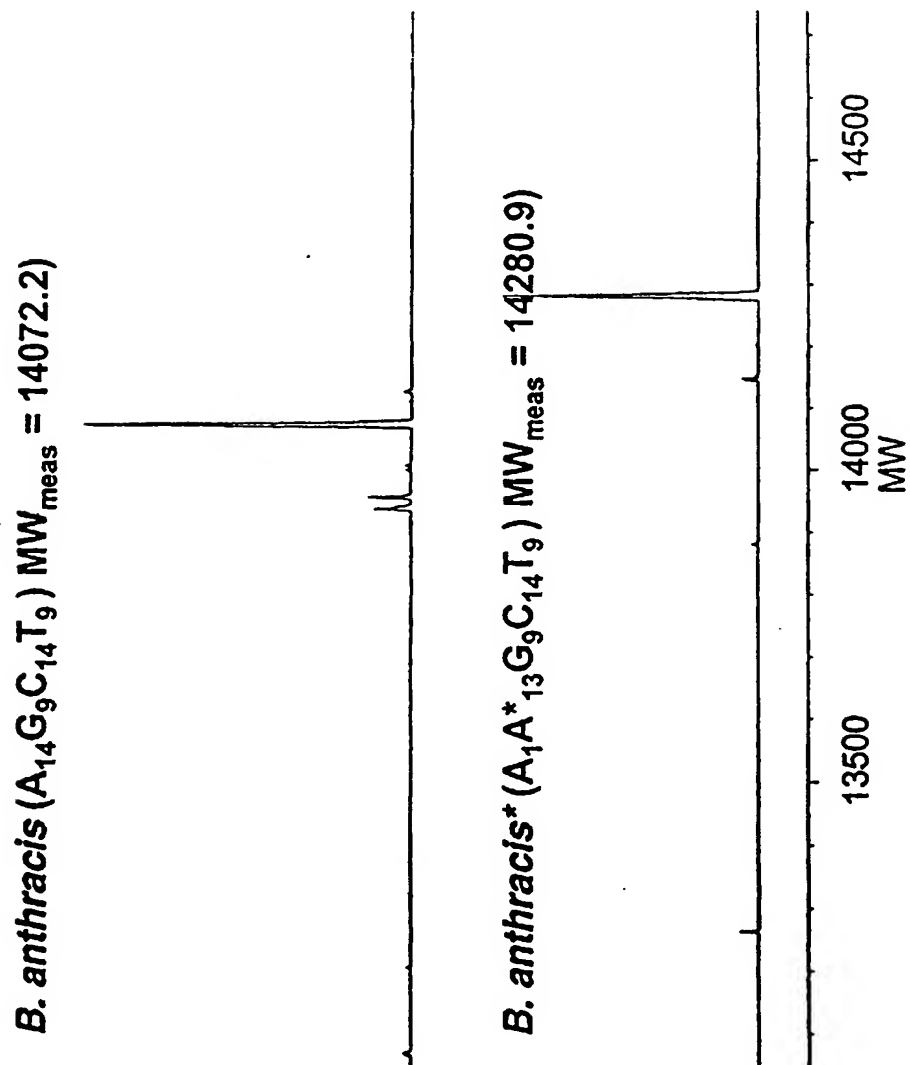


FIG. 6

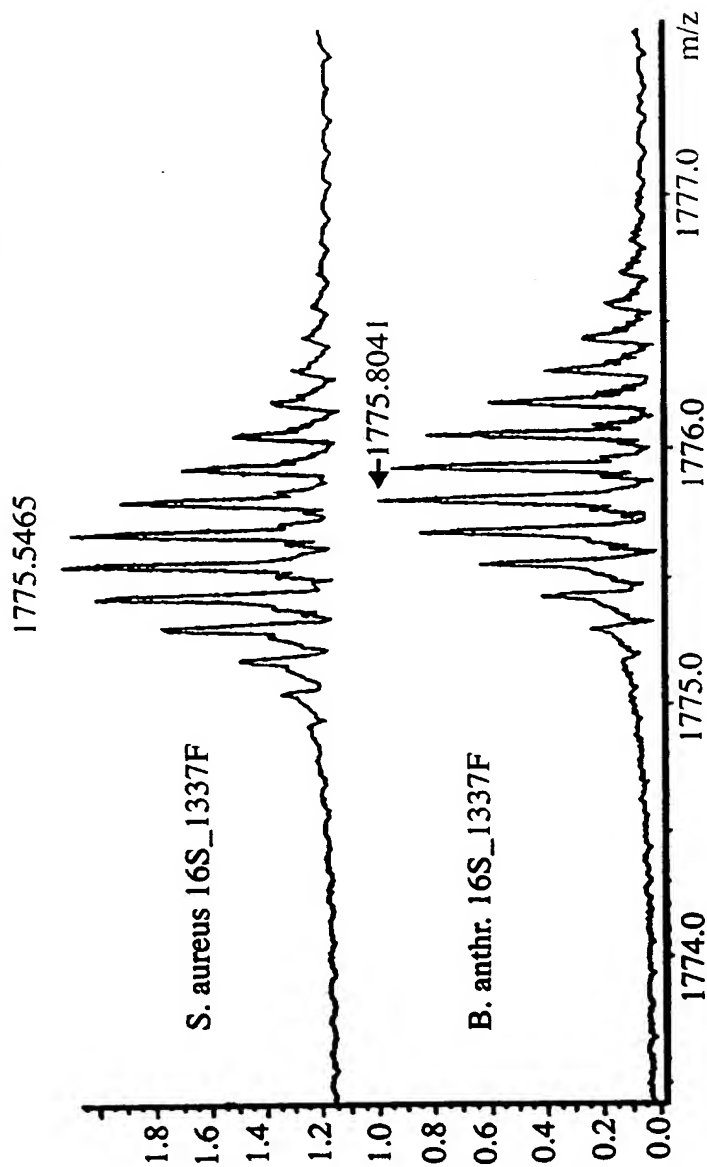


FIG. 7

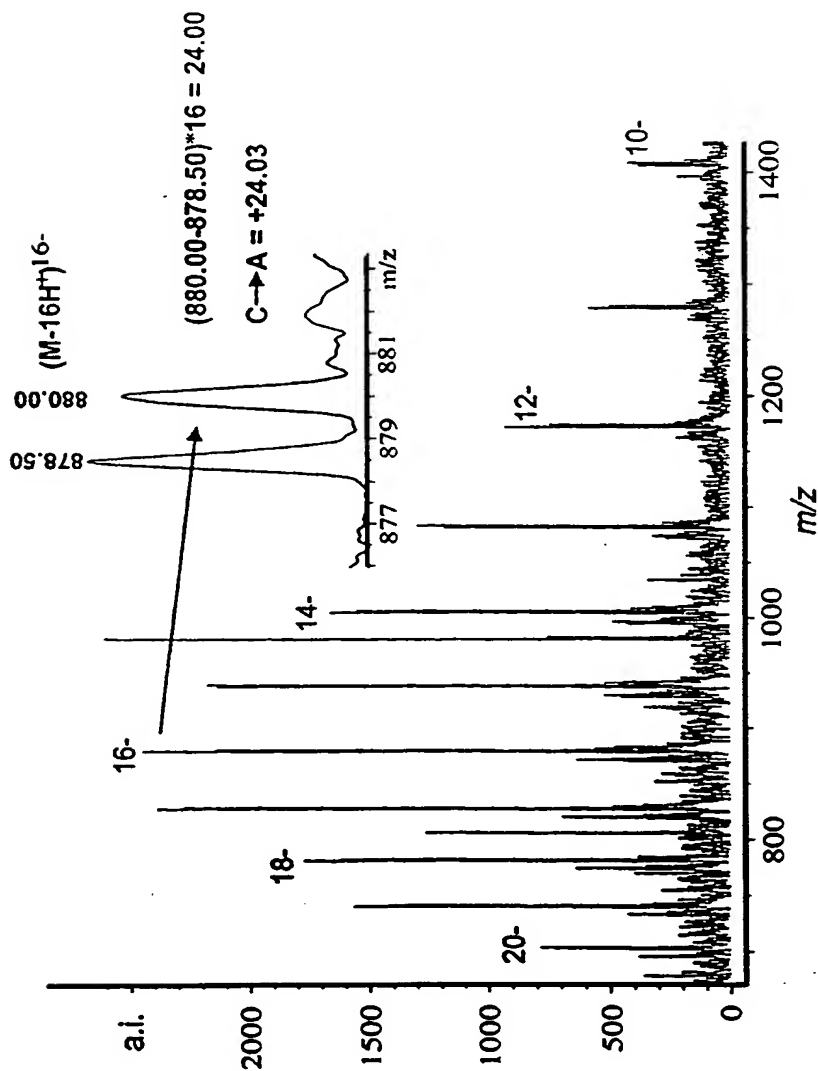


FIG. 8

ESI-TOF MS of sspE 56mer + Calibrant

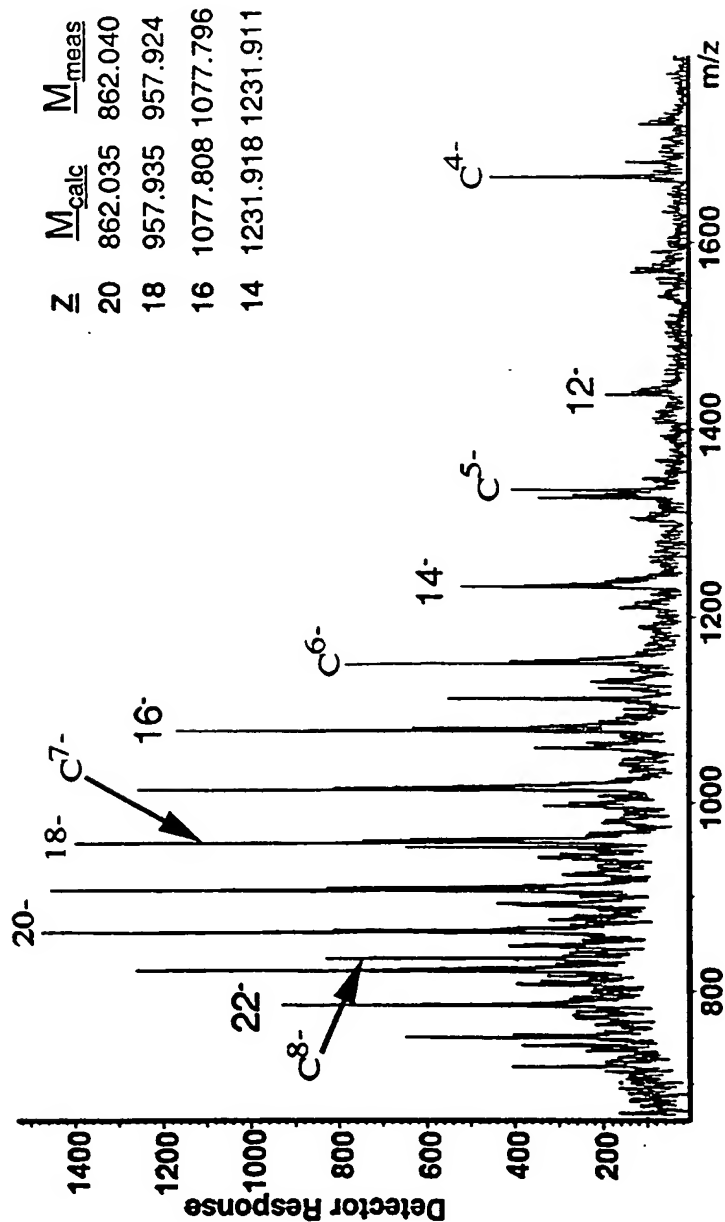


FIG. 9

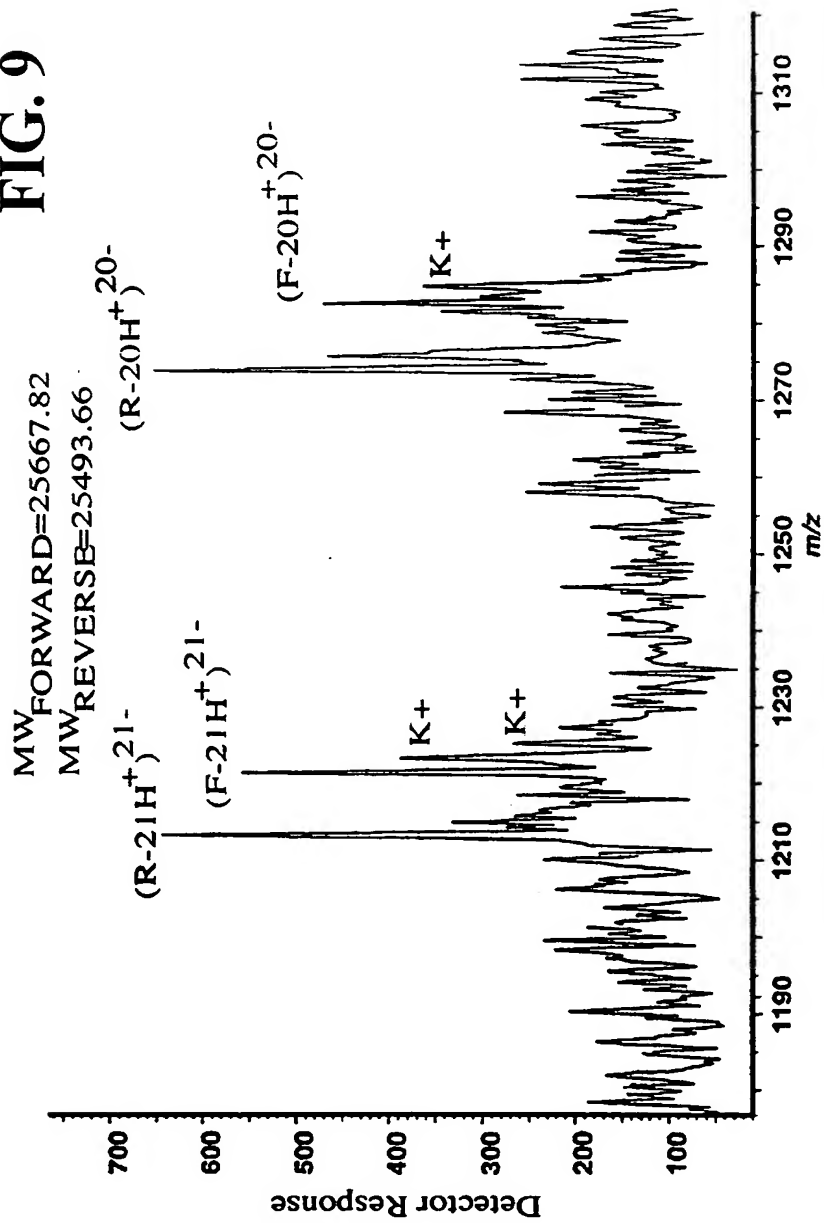


FIG. 10

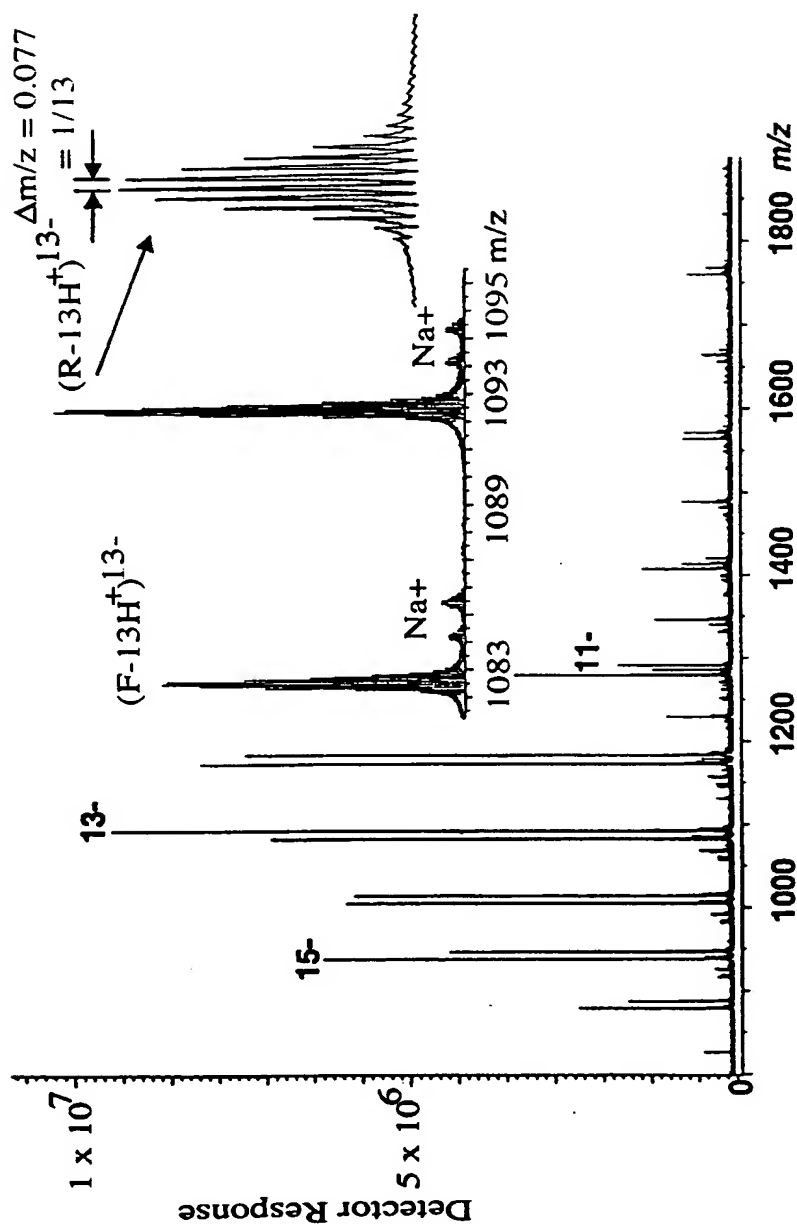


FIG. 11

